

FIG. 1A
(Prior Art)

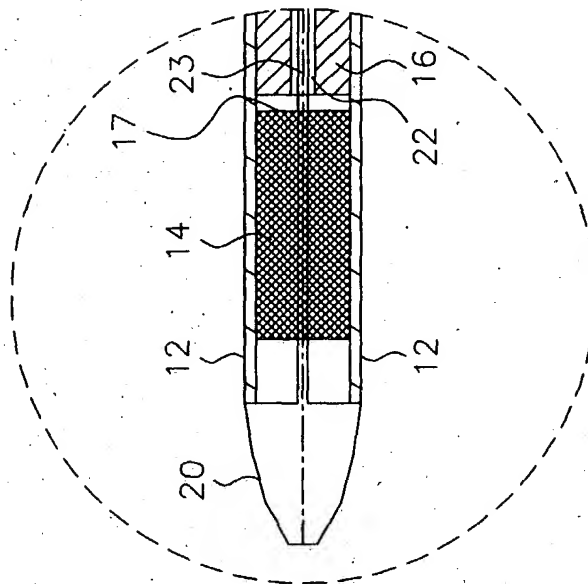


FIG. 1B
(Prior Art)

1/6

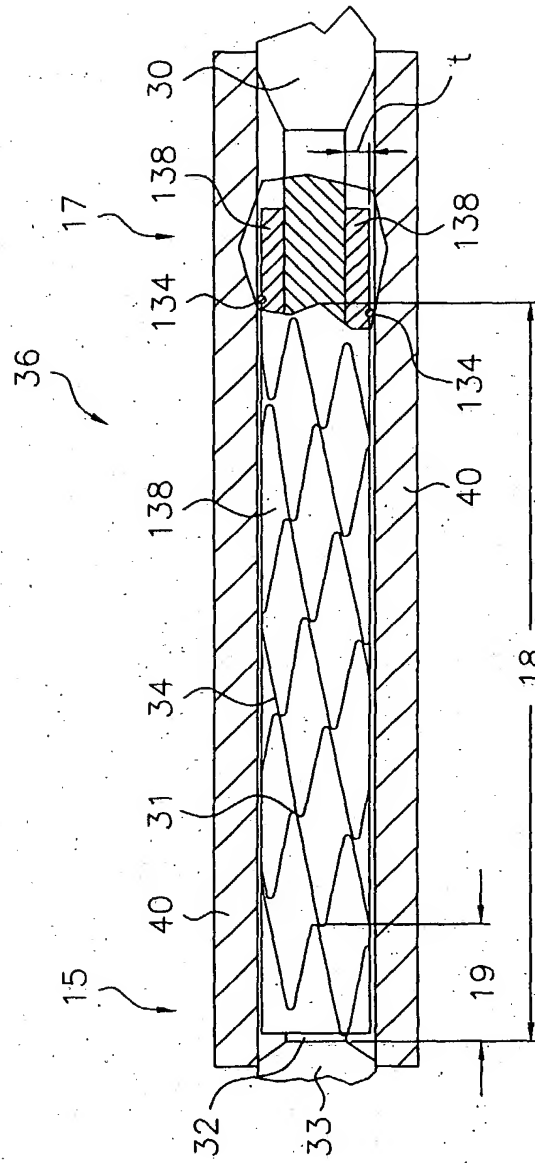


FIG. 2A

2/6

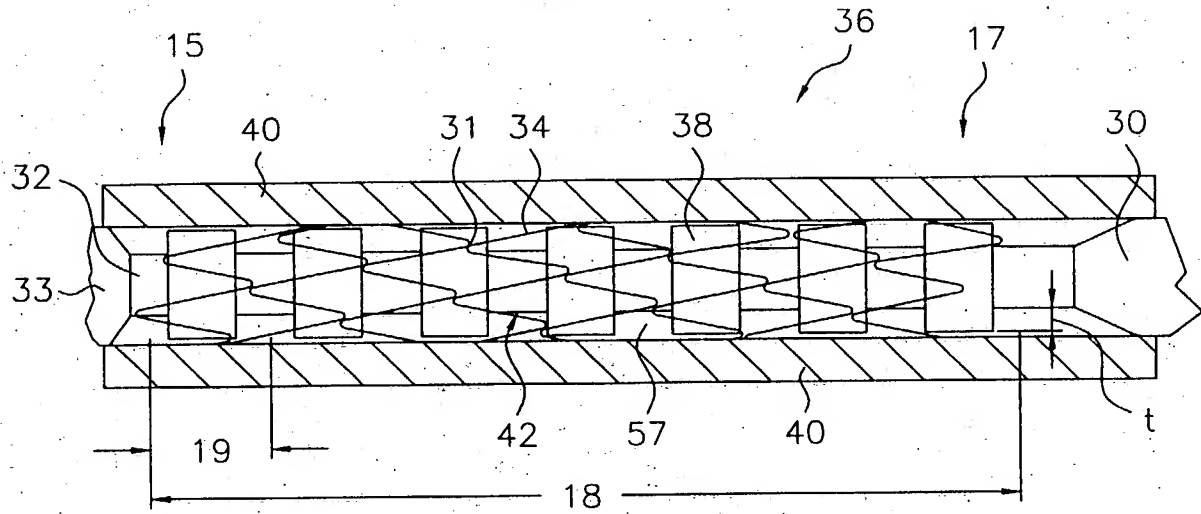


FIG. 2B

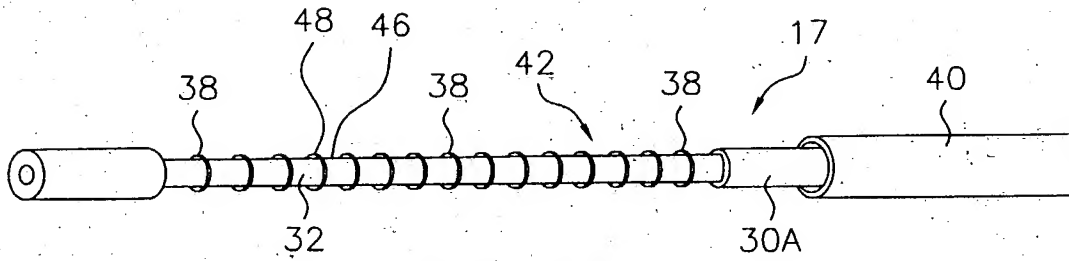


FIG. 3A

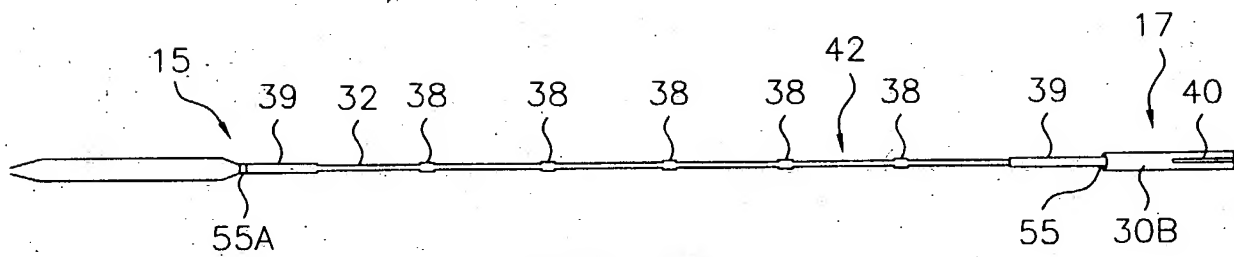


FIG. 3B

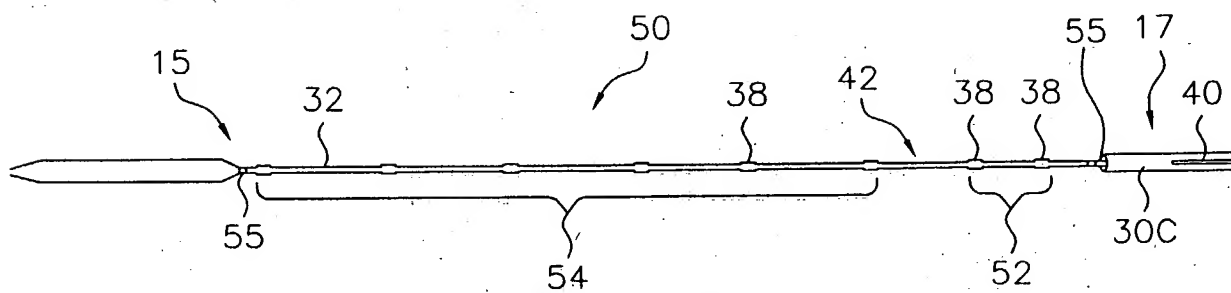


FIG. 3C

3/6

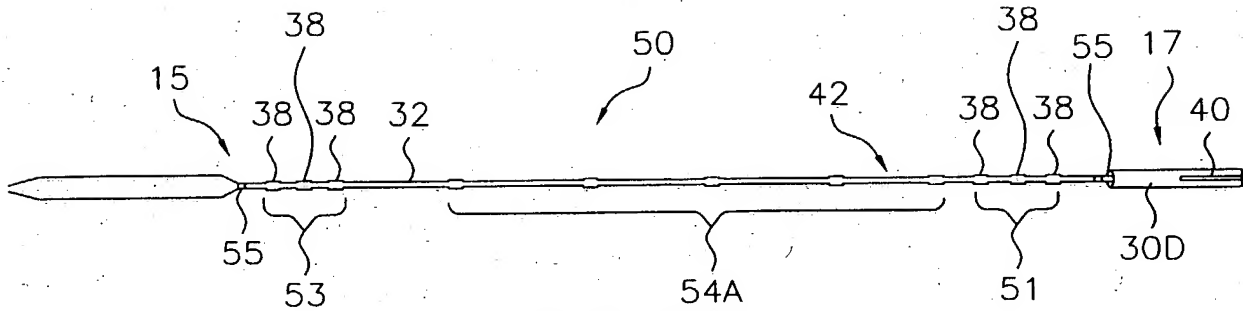


FIG. 3D

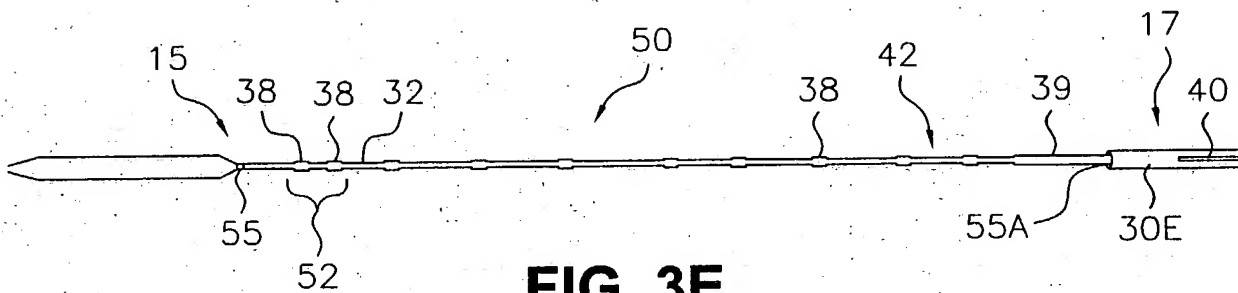


FIG. 3E

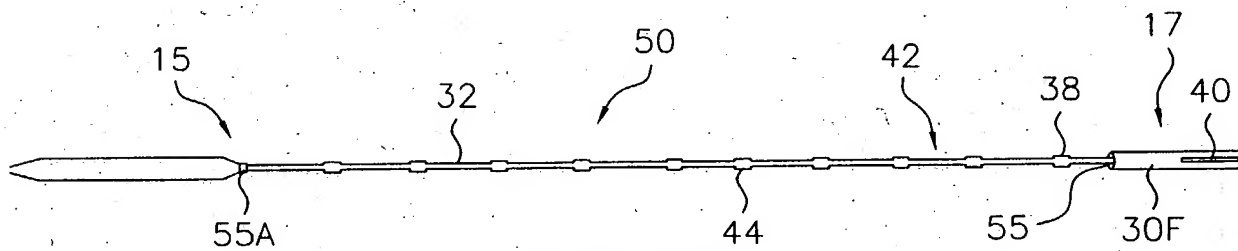


FIG. 3F

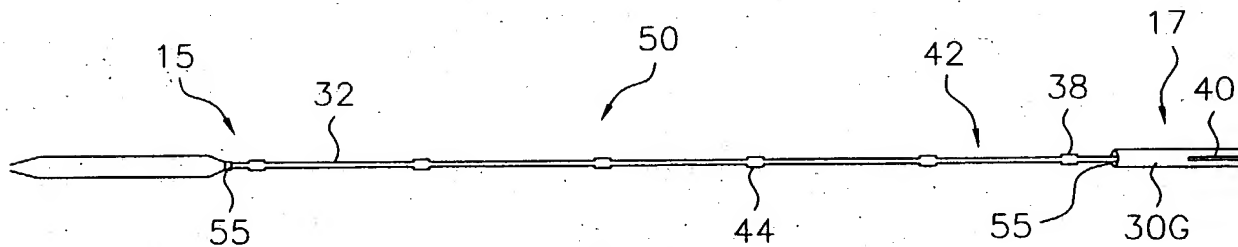


FIG. 3G

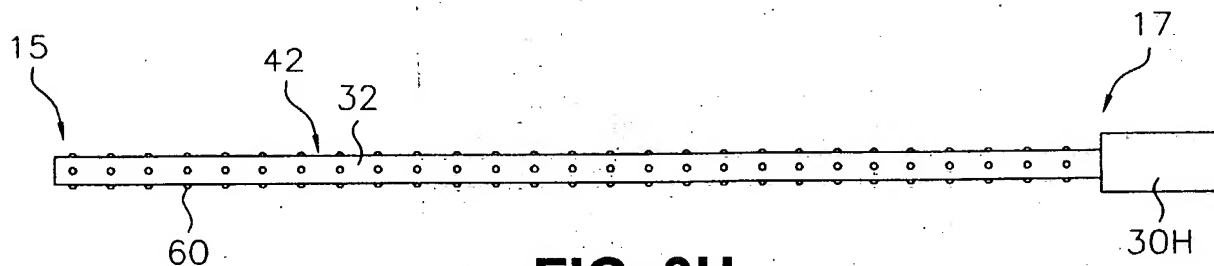


FIG. 3H

4/6

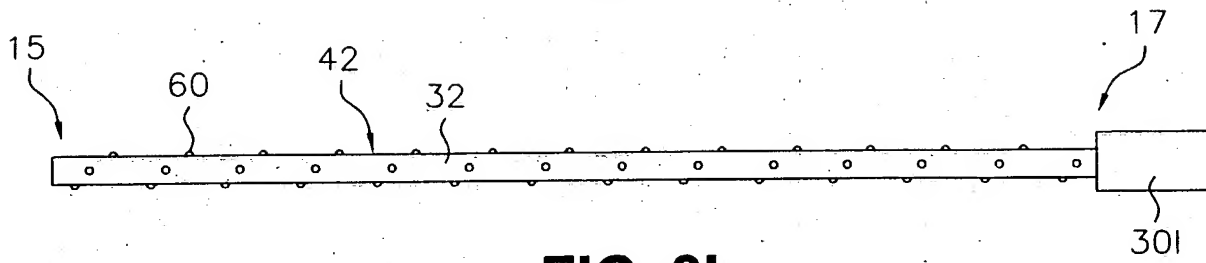


FIG. 3I

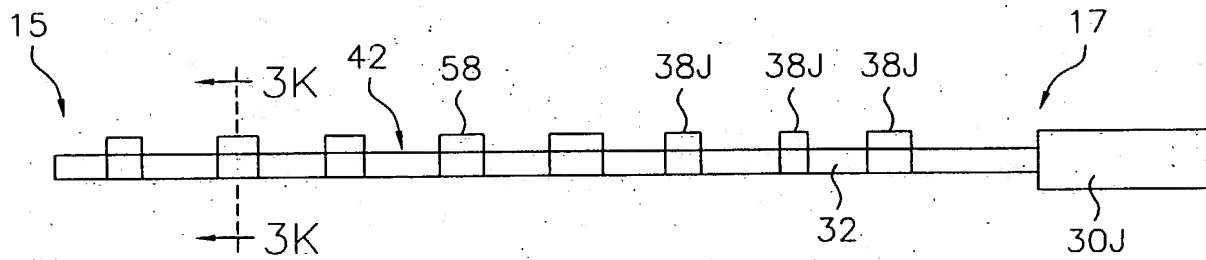


FIG. 3J

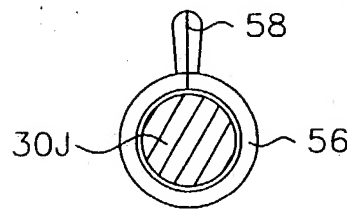


FIG. 3K

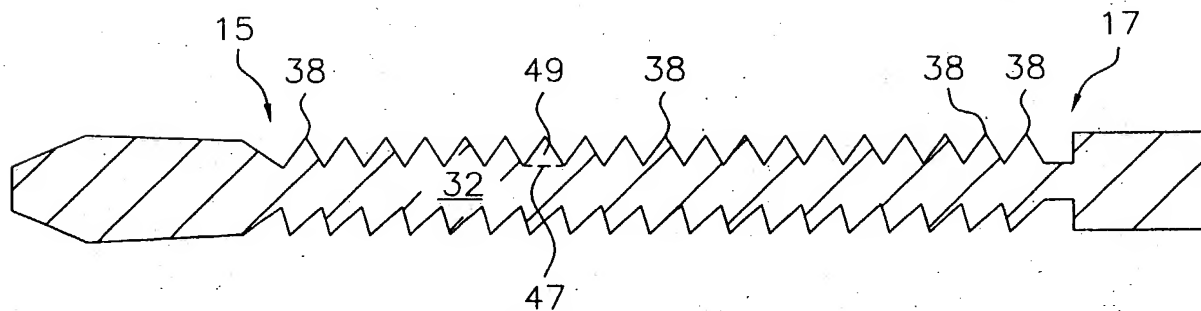


FIG. 4A

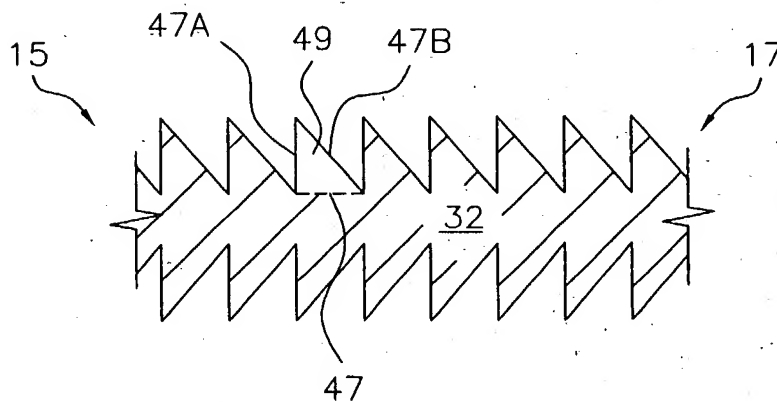


FIG. 4B

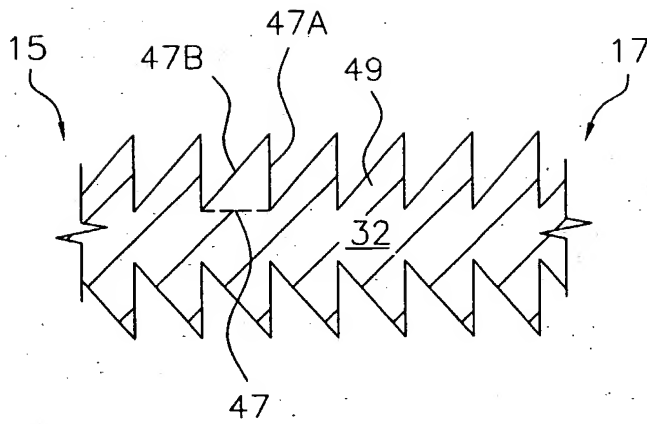


FIG. 4C

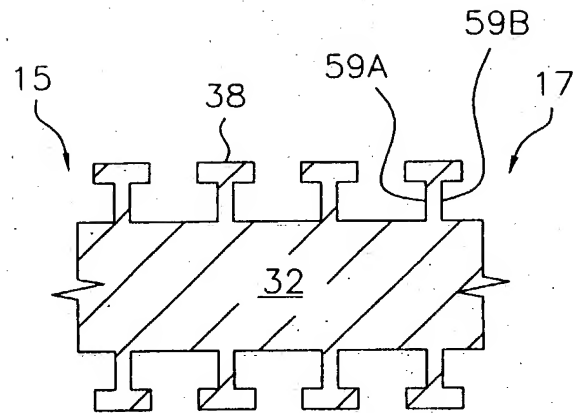


FIG. 4D

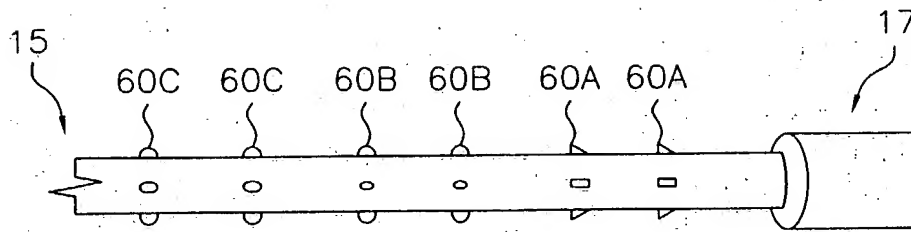


FIG. 5

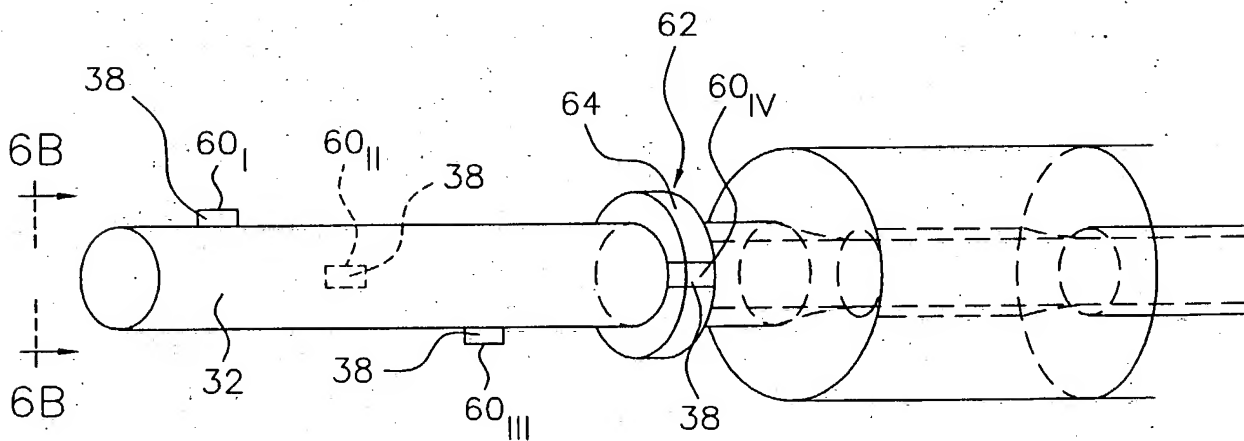


FIG. 6A

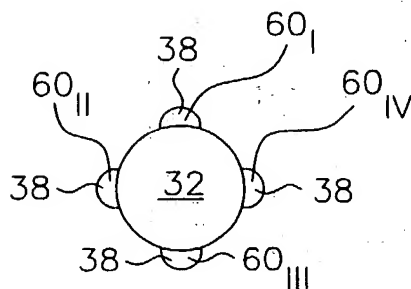


FIG. 6B

FIG. 1 is a perspective view of a medical device 15. The device includes a handle 30 with a trigger 32, a shaft 17, and a distal tip 33. A section of the shaft is labeled 138.

FIG 9A

FIG. 9C